

APPROVAL
EC Directive 93/42/EEC Annex V, Article 3
Quality Assurance System Production

Registration No.: DD 60024356 0001

Report No.: 15030231 001

Manufacturer: Hangzhou Hua'an Medical &
Health Instruments Co., Ltd.
Building 2, Baimiao Ind. Park
Economic Develop. Zone Wuchang

Hangzhou, Zhejiang 310023
China


Scope: Manufacture of Digital Thermometers, Infra-red Ear
Thermometers, Digital Blood Pressure Monitors
(Digital Sphygmomanometers)

Replaces Approval, Registration No.: DD 60008079 0001

Date of Expiry: 24.02.2014

The Notified Body hereby authorizes the quality management system established and applied by the company mentioned above. The requirements of Annex V, Article 3 of the directive have been met. This approval is subject to periodic surveillance, defined by Annex V, Article 4 of the aforementioned EC Directive, and can be used by the company with the manufacturer's declaration of conformity.

Cologne, 25.02.2009

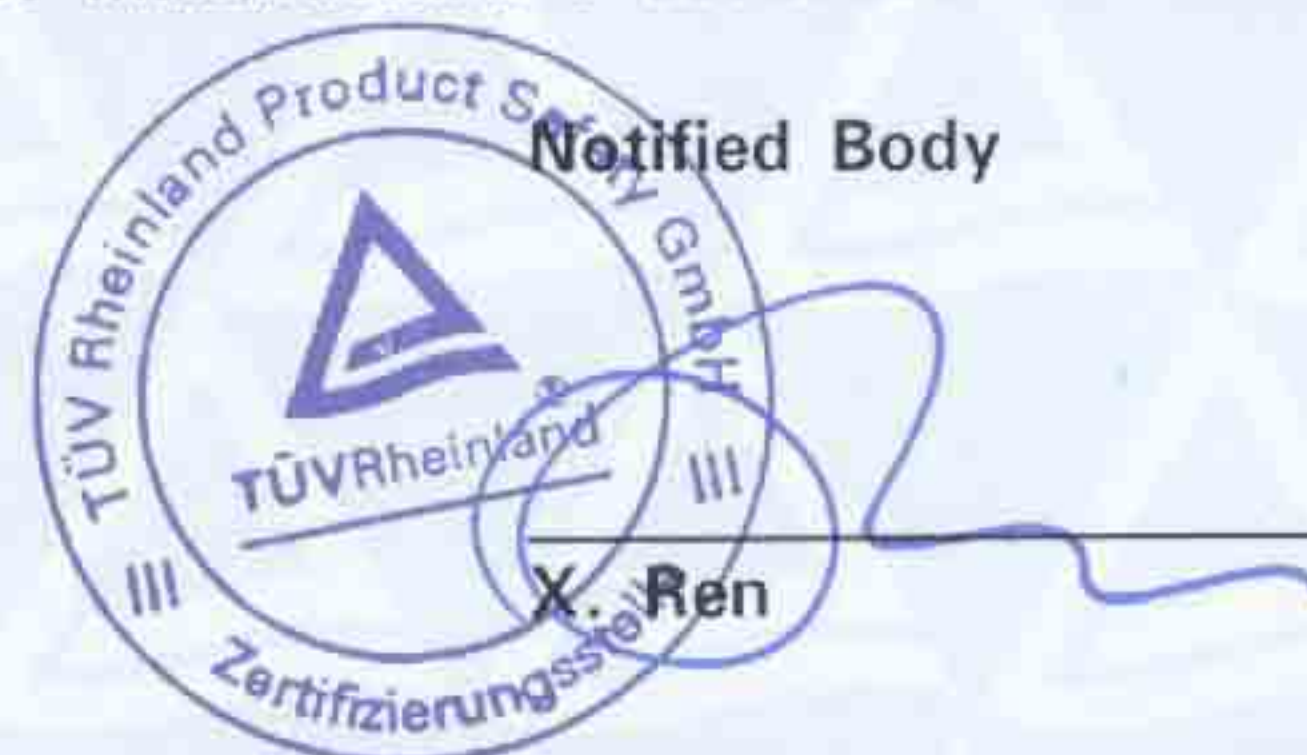

TÜV Rheinland Product Safety GmbH - Am Grauen Stein - D-51105 Köln
Accredited by Zentralstelle der Länder für Sicherheitstechnik (ZLS) and
Zentralstelle der Länder für Gesundheitsschutz bei Arzneimitteln und Medizinprodukten (ZLG).

Notified under No. **0197** to the EC Commission.

CE The CE marking may be used if all relevant and effective EC Directives are complied with. CE